

Sample Received: **April 15, 2026** COA Issued: **June 9, 2026**

PRODUCT INFORMATION

Vendor:	Sample Name:	Sample Type:	Lot Number:	MW (g/mol):
Neurovia	Tesofensine	Capsule	TESOCAP4-2026-MG	328.3



ANALYTICAL METHODS

Identity: Confirmed via MALDI-MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation

TEST RESULTS

Specification	Result	Method	Status
Identity: Tesofensine	Tesofensine	MALDI-MS	✓ Conforms
Content		HPLC Quantitation	✓ Conforms
Overall Purity	99.8%	RP-HPLC (214 nm)	✓ Conforms
Endotoxin	<0.05 EU/mL	<USP 85>	✓ Conforms
Heavy Metals	<0.001 ppm	<USP232>	✓ Conforms

HPLC Chromatogram (Retention Time: 9.358 min)

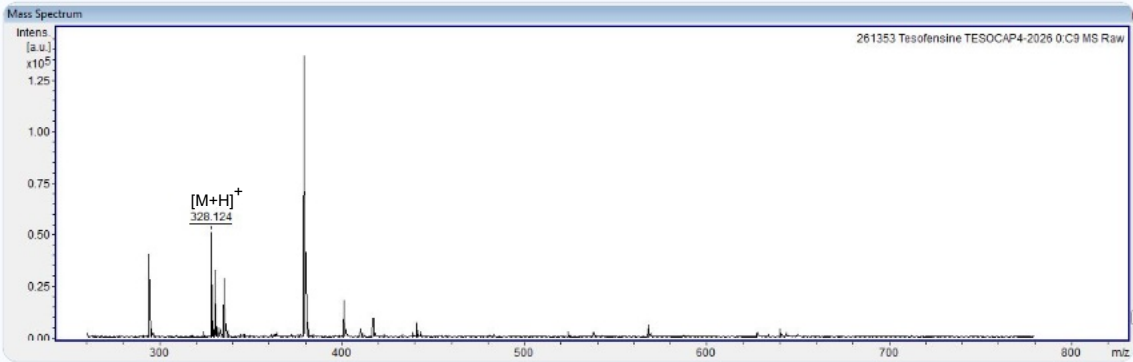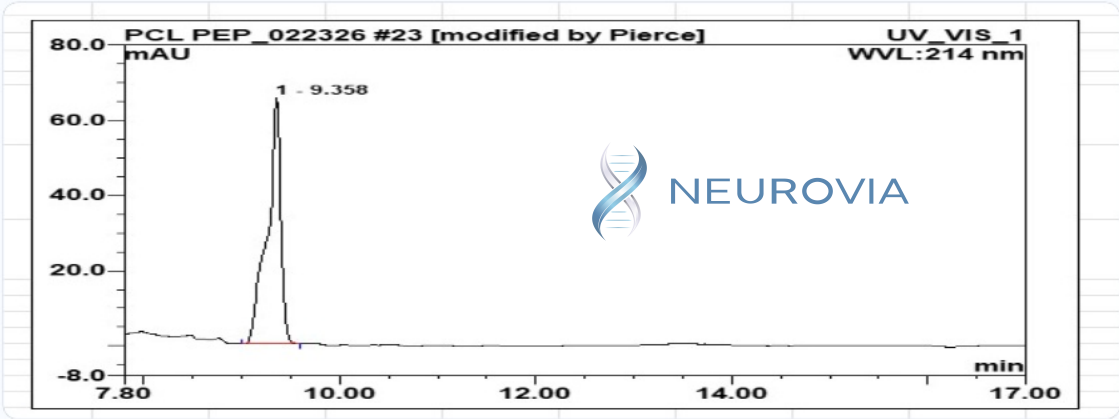

Certification: This COA confirms that the tested material meets or exceeds Bioviridian’s analytical quality specifications for peptide research use.
Visit: <https://bioviridians.com/coa-search.html>



Shane Straight
Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.