

Sample Received: April 15, 2026

COA Issued: June 9, 2026

PRODUCT INFORMATION

Vendor: **Neurovia** Sample Name: **Thermox** Sample Type: **Capsule** Lot Number: **THERMAP1-2026** MW (g/mol): **290.3, 340.3**

ANALYTICAL METHODS

Identity: Confirmed via MALDI-MS



Purity: RP-HPLC (214 nm)

Content: HPLC quantitation

TEST RESULTS

Specification	Result	Method	Status
Identity: Thermox (BAM-15, SLU-PP-332, CTS	BAM-15, SLU-PP-332	MALDI-MS	✓ Conforms
Content		HPLC Quantitation	✓ Conforms
Overall Purity	99.7%	RP-HPLC (214 nm)	✓ Conforms
Endotoxin	<0.05 EU/mL	<USP 85>	✓ Conforms
Heavy Metals	<0.001 ppm	<USP232>	✓ Conforms

HPLC Chromatogram (Retention Time: 9.358 min)

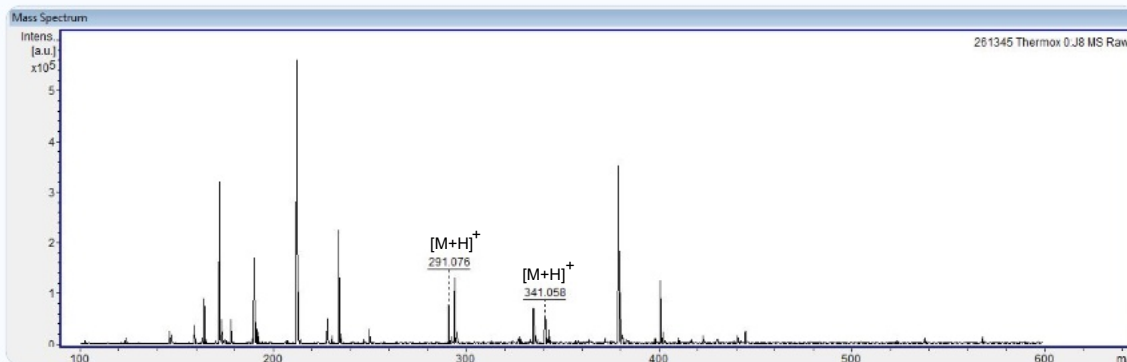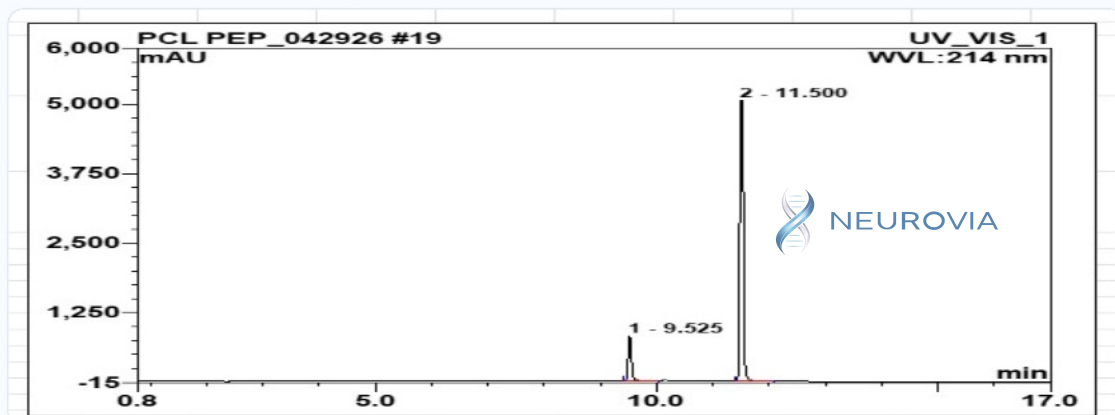

Certification: This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Visit: <https://bioviridians.com/coa-search.html>*Shane Straight*Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.